

Fine optimization of a dissolution-DNP experimental setting for ^{13}C NMR of metabolic samples

Arnab Dey¹, Benoît Charrier¹, Karine Lemaitre¹, Victor Ribay¹, Dmitry Eshchenko^{2a}, Marc Schnell^{2a}, Roberto Melzi^{2b}, Quentin Stern³, Samuel F. Cousin⁴, James G. Kempf^{2c}, Sami Jannin³, Jean-Nicolas Dumez¹, Patrick Giraudeau¹

¹Nantes Université, CNRS, CEISAM UMR 6230, F-44000 Nantes, France.

²Bruker Biospin, ^aIndustriestrasse 26, 8117 Fällanden, Switzerland, ^bViale V. Lancetti 43, 20158 Milano, Italy, ^c15 Fortune Dr., Billerica, MA 01821 USA

³Université de Lyon, CNRS, Université Claude Bernard Lyon 1, ENS de Lyon, Centre de RMN à Très Hauts Champs (CRMN), UMR5082, F-69100 Villeurbanne, France.

⁴Aix Marseille Univ., CNRS, ICR, 13397, Marseille, France

Correspondence to: Patrick Giraudeau (patrick.giraudeau@univ-nantes.fr)

Abstract. NMR based analysis of metabolite mixture provides crucial information on biological systems but mostly [rely-relies](#) on ID ^1H experiments for maximizing sensitivity. However, strong peak overlap of ^1H spectra often is a limitation for the analysis of inherently complex biological mixtures. Dissolution Dynamic Nuclear Polarization (d-DNP) improves NMR sensitivity by several orders of magnitude, which enables ^{13}C NMR based analysis of metabolites at natural-abundance. We have recently demonstrated the successful introduction of d-DNP into a full untargeted metabolomics workflow applied to the study of plant metabolism. Here we describe the systematic optimization of d-DNP experimental settings for experiments at natural ^{13}C abundance, and show how the resolution, sensitivity, and ultimately the number of detectable signals improve as a result. We have systematically optimized the parameters involved (in a semi-automated prototype d-DNP system, from sample preparation to signal detection, aiming at providing an optimization guide for potential users of such system who may not be experts in instrumental development). The optimization procedure makes it possible to detect previously inaccessible protonated- ^{13}C signals of metabolites at natural abundance with at least 4 times improved line shape and a high repeatability compared to a previously reported d-DNP enhanced untargeted metabolomic study. This extends the application scope of hyperpolarized ^{13}C NMR at natural abundance and paves the way to a more general use of DNP-hyperpolarised NMR in metabolomics studies.

1. Introduction

NMR spectroscopy offers [unparalleledunparallel](#) robustness and reproducibility for the analysis of complex metabolite mixtures. Such advantages make NMR an ideal tool for a number of analytical applications such as targeted or untargeted metabolomics, stable-isotope resolved studies of metabolism, pharmacokinetic studies, bioprocess optimization (Zhang et al., 2010; Wang et al., 2013; Zhang et al., 2008; Calvani et al., 2010; Liu et al., 2010; Strickland et al., 2017; Emwas et al., 2019; Kim et al., 2013; Wishart, 2008) etc. However, NMR suffers from poor sensitivity which limits the detection of metabolites to the micromolar concentration range (in contrast, the limit of detection of

35 mass spectroscopy can reach sub-nanomolar concentrations(Grotti et al., 2009; Liem-Nguyen et al., 2015; Li et al.,
2020). Owing to such challenge, the analysis of metabolic mixtures by NMR mostly relies on ¹H spectroscopy, which
is, however, often marred by the strong signal overlap in ¹H spectra of complex biological sample due to limited
spectral dispersion. ¹³C NMR could be a promising solution as it offers wide spectral dispersion which results in a
better separation of metabolite signals. At present, the application of ¹³C NMR to metabolite mixtures at natural
40 abundance is limited due to about 2900-fold reduced sensitivity (owing to its low natural abundance and gyromagnetic
ratio) versus ¹H. Therefore, to expand the applicability of ¹³C NMR metabolomics it is of much interest to develop
methods which improve the sensitivity of ¹³C signal detection while retaining its resolution advantage. Indeed,
detecting major metabolites in biological samples at natural abundance would require reaching SNR values above 10
for mM concentrations or less, which is not possible with conventional hardware. The development of home-made ¹³C
45 optimized NMR probes for metabolomics has been shown to yield improved accuracy in the metabolite identification
and group separation for mass limited samples(Clendinen et al., 2014). However, the ¹³C signal sensitivity generally
remains too low for routine metabolomics applications and further development is required to improve sensitivity.
Hyperpolarization techniques are in the forefront among such developing methods. Hyperpolarization stems from
creating a far from equilibrium spin population distribution which results in a significant increase of the nuclear spin
50 polarization compared to thermal equilibrium values, leading to considerable improvement in sensitivity. Several
hyperpolarization techniques such as Dissolution Dynamic Nuclear Polarization (DNP)(Jannin et al., 2019; Giraudeau
et al., 2009; Singh et al., 2021a; Dey et al., 2020; Guduff et al., 2017; Leon Swisher et al., 2015; Dumez et al., 2015),
ParaHydrogen-Induced Polarization (PHIP)(Kiryutin et al., 2019; Ivanov et al., 2009), and its reversible version, Signal
Amplification by Reversible Exchange (SABRE)(Lloyd et al., 2012; Daniele et al., 2015; Eshuis et al., 2014; Guduff
55 et al., 2019)have been implemented successfully for the analysis of complex mixtures. Among all the hyperpolarization
techniques, dissolution ~~state~~-DNP (d-DNP) is of particular interest for metabolic mixtures as it has been known to
improve the signal sensitivity by more than 10,000 times in a non-selective fashion (Ardenkjær-Larsen et al., 2003).
In d-DNP, nuclear spins are polarized in the solid-state at cryogenic temperatures (typically 1-2 K), in a high magnetic
field (3-7 T), by microwave irradiation in the presence of a radical species. This is followed by rapid dissolution and
60 transfer of the sample to a nearby NMR spectrometer where hyperpolarized signals are acquired at room temperature
in the liquid-state. Despite offering impressive sensitivity improvements, the instrumental complexity of d-DNP could
appear contradictory with the high-throughput, precision and robustness needed for analytical applications. However,
several recent studies highlighted the potential of d-DNP for analyzing complex metabolic mixtures by ¹³C NMR.
Lerche et al. demonstrated the relevance of d-DNP for fluxomic studies by quantifying the ¹³C isotopic patterns to
65 understand the metabolic activity of cancer cell extract incubated with ¹³C-enriched glucose(Frahm et al., 2021; Lerche
et al., 2018; Frahm et al., 2020). Recent investigations also focused on the development of d-DNP methods to analyze
metabolic samples at natural ¹³C abundance, taking advantage of ¹H → ¹³C cross polarization (CP) in the solid-state to
reach high ¹³C polarization levels in a short time(Batel et al., 2014; Bornet et al., 2013). In 2015, we showed that d-
DNP could be used to detect metabolites of plant and cell extracts at ¹³C natural abundance,(Dumez et al., 2015) and
70 we then reported that the repeatability of this approach was compatible with metabolomics applications(Bornet et al.,
2016).

In a recent proof-of-concept study, we demonstrated that d-DNP could be incorporated into a full untargeted metabolomics workflow capable of separating tomato extract samples at two different ripening stages and of highlighting corresponding biomarkers (Dey et al., 2020). In this study, we described preliminary experimental optimizations that played a key role to achieve the precision needed for the application of d-DNP to a series of metabolic samples. These included the use of an Hellmanex™ coated NMR tube which helps to reduce the formation of microbubbles due to the rapid motion of the dissolved sample inside the NMR tube. Moreover, we showed that with the use of an appropriate internal standard, the effect of instrumental variability on relative signal quantification could be reduced from about 10% to 3%. Overall, the study showcases the potential of d-DNP for metabolomics. However, this study also highlighted that a full utilization of the prototype-DNP setting for such application would require a thorough optimization of several experimental parameters. Such optimization was beyond the scope of that report owing to the large number, complexity and inter-dependence of parameters involved in the d-DNP setting. A recent review by Elliott et al. (Elliott et al., 2021) ~~provided~~ provides a detailed description of the practical aspects of the d-DNP workflow, highlighting the good experimental practices that ensure optimized sensitivity and line shape on the resulting liquid-state spectra. In the perspective of applying d-DNP to complex diluted mixtures of metabolites at ¹³C natural abundance, a particular focus should be made on the experimental parameters that impact sensitivity and repeatability, two key ingredients for analytical applications. Such optimization should also be oriented towards potential users of this equipment who may not be experts in instrumental development.

In this context, the present study demonstrates a systematic optimization of a prototype d-DNP setting focusing on the parameters which could be tuned by the user without the need of instrumental development. More specifically, we present the results of a fine optimization of d-DNP settings for the analysis of metabolic mixtures at ¹³C natural abundance, showcasing a significant improvement (about 5 times in the quaternary ¹³C region and 50 times in protonated ¹³C region) in sensitivity compared to our previous study, while preserving a high repeatability. We also intend this optimization procedure to serve as a guideline for the various applications of d-DNP in the field of analytical chemistry.

2. Design of Experiment

A brief schematic description of the d-DNP experimental setting is presented in Figure 1 highlighting the most important components ~~as well as, the~~ The figure represents the operational workflow indicating important steps in sequence. The complete d-DNP operation is divided into 4 main experimental steps *i.e.* sample preparation, polarization in the solid-state, dissolution and transfer, and signal acquisition in the liquid-state. In the operational workflow, we have schematically indicated the change of several relevant parameters as experienced by the sample during the d-DNP experiment.

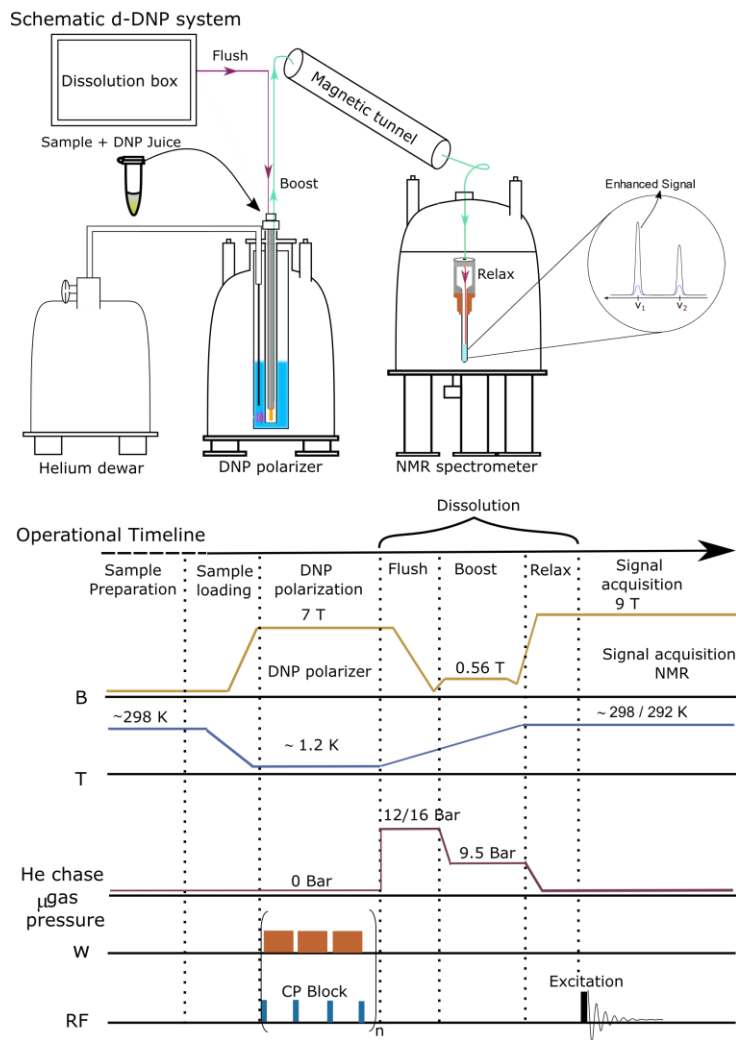


Figure 1. Schematic description of the semi-automated prototype dissolution DNP system along with operational timeline indicating important events during d-DNP operation in sequence

Table 1. List of parameters for the plan of optimization of DNP setting. PA: polarizing agent. CP: cross-polarization. μ w: microwaves. VTI: variable temperature insert (Enclosure where the sample is vitrified, hyperpolarised and dissolved at cryogenic temperature).

| | A. Sample Preparation | B. DNP Polarization | C. Dissolution | D. Signal Acquisition |
|---------------------------------|---|---|---|---|
| Parameters Optimized | <ol style="list-style-type: none"> 1. PA concentration 2. DNP juice composition and order of mixing 3. Ripening time (R_T) 4. Sample Sonication parameters | <ol style="list-style-type: none"> 1. μw parameters 2. ^1H DNP build up 3. CP parameters 4. Vitrification parameters | <ol style="list-style-type: none"> 1. Dissolution solvent (CD_3OD, D_2O) 2. Dissolution duration 3. Sample transfer line | <ol style="list-style-type: none"> 1. Pre-shimming & Pre-tuning |
| Parameters not Optimized | <ul style="list-style-type: none"> • Choice of PA • Thermal history of the sample | <ul style="list-style-type: none"> • VTI temperature & pressure stability • Field strength of the DNP polarizer • μw source | <ul style="list-style-type: none"> • Dissolution solvent volume • Dissolution temperature & pressure • Other dissolution solvent • Other sample transfer methods | <ul style="list-style-type: none"> • Standard ^{13}C NMR parameters (pulse length, power, decoupling...) |

110 Table 1 provides a list of all parameters involved in the workflow indicating those to be optimized from a practical user viewpoint without the expertise of hardware development. In the next section, we qualitatively describe all the relevant parameters involved in DNP experimental setting and ~~identified-identify~~ the parameters which could potentially impact the analytical performance of the d-DNP workflow for the analysis of metabolic mixtures at natural ^{13}C abundance.

115 Most of these parameters are interdependent. Therefore, instead of a sequential, one-by-one optimization of these parameters, the ideal strategy would consist in testing all (or many) possible parameter combinations. However, it would require a number of experimental attempts that would be unrealistic with respect to the liquid Helium consumption, considering that 3 experiments for each condition would be required to evaluate the repeatability. Therefore, we have divided all the parameters into 4 main operational subunits that we optimized in two layers *i.e.*: i) 120 a systematic investigation with no repetition to find out the optimum combinations of impactful parameters on a sensitivity basis, ii) an evaluation of the repeatability on the basis of three experiments for the most sensitive conditions.

3. Experiments and parameters

In this section, we sequentially describe the different steps of the experiment, highlighting the key parameters in the perspective of application to the sensitive and repeatable analysis of metabolite mixtures at natural ^{13}C abundance.

125

A. Sample preparation

The d-DNP sample preparation procedure is essential to enable uniform nuclear spin polarization across the sample at a cryogenic temperature, which in turn affects the achievable sensitivity and repeatability (El Daraï and Jannin, 2021). A standard sample preparation protocol is required with a careful choice of parameters. Based on previous d-DNP studies and on our own experience, we identified three potentially important parameters that could impact the d-DNP workflow and should be optimized: “DNP juice” composition, ripening time, and Polarizing agent (PA) concentration (Plainchont et al., 2018; Köckenberger, 2014; Elliott et al., 2021). For the experimental optimization and evaluation of the d-DNP workflow, a mixture of three common metabolites at natural ^{13}C abundance (alanine, sodium acetate, sodium pyruvate) was prepared, each at a 5 mM concentration, which is representative of the concentration of major metabolites in extracts. Sodium 3-trimethylsilylpropionate-d4 (Na-TSP-d4; 98% D; 20 mM) was added as an internal standard, as previously reported (Dey et al., 2020). For DNP experiments, these chemicals were dissolved in a glassy matrix along with the polarizing agent (PA), 4-hydroxy-2,2,6,6-tetramethylpiperidine-1-oxyl (TEMPOL). To ensure optimal solubility, samples were stirred for 60 s with a mechanical stirrer. Sample sonication was also evaluated by sonicating the sample for 60 s before inserting the sample into the polarizer, but it did not impact the polarization efficiency.

For the whole study, samples were prepared from the same stock solution to avoid unwanted variation from the differences in sample measurement. The stock solution was prepared by solubilizing the metabolites and TEMPOL in the DNP juice, then DNP samples were equally divided and stored inside a -80°C freezer. Before the start of the polarization experiment, samples were taken out from the freezer and stirred at room temperature as mentioned above, then transferred into the sample cup. Care should be taken to avoid small bubbles and residue of sample droplets residing in the top part of the sample cup which is above the active μw irradiation region. The sample cup was then vitrified at ca. 4 K inside the polarizer.

It is also important to trace the amount of sample (in weight) taken inside the sample cup before hyperpolarization. In our case, 200 μl of DNP sample weighted 258 mg with a standard variation of 1% of all the samples used for experiments. Also, we have monitored the ^1H signal integral without microwave at solid state to investigate the variation of signal integral without microwave. It is important to note that such signal integral differs from the actual thermal signal of the sample as the acquired signal integral includes the background signal from the sample cup. In the following section, we discuss the key parameters involved in sample preparation for d-DNP experiments.

A.1 PA concentration

The PA plays a central part in DNP polarization. A broad variety of PA is available depending on the targeted sample and application. It has been well discussed in several studies that nitroxide-based radicals such as TEMPOL are preferred for $^1\text{H} \rightarrow ^{13}\text{C}$ CP based d-DNP, as the broad EPR line width of TEMPOL ensures high and rapid ^1H polarization, which in turn is the main source of ^{13}C polarization. Therefore, TEMPOL was chosen as a PA for this study. A range from 25 – 100 mM concentration of TEMPOL has been previously investigated (Elliott et al., 2021). For the application to metabolite mixtures at natural ^{13}C abundance, the TEMPOL concentration should be optimized

Mis en forme : Exposit

to achieve the highest DNP polarization through a rapid DNP build up with minimal contribution to the polarization losses during sample transfer before liquid-state signal acquisition.

A.2 “DNP juice” composition and order of mixing

165 The DNP juice composition consists of a mixture of glycerol, D₂O, H₂O, which ensures a uniform distribution of
analytes and polarizing agent (PA) forming a glassy sample at cryogenic temperatures (about 1-2 K). Previous studies
reported that the efficiency of DNP juice particularly depends on the nature and concentration of PA (Leavesley et al.,
2018a). Several studies reported that a glycerol content > 55% was sufficient to form a glass at 1-2 K (Puzenko et al.,
2005; Leavesley et al., 2018; Hayashi et al., 2005). However, very high percentage of glycerol in the “DNP juice”
170 restricts the solubility of the biological sample in the DNP juice. Previous DNP studies reported up to 60% of glycerol
content in the DNP juice composition (Jähnig et al., 2019; Tran et al., 2020; Overall and Barnes, 2021; Kaushik et al.,
2022). Care should be taken to decide the order of mixing the sample in H₂O-D₂O and glycerol of DNP juice depending
on the solubility in H₂O-D₂O compared to glycerol for ensuring complete solubility of sample in DNP juice.

A.3 Ripening time

175 A recent study reported that following the completion of DNP sample preparation, a delay before vitrification (ripening
time) could lead to the formation of nanoscopic water vesicles in a glycerol rich matrix, resulting in an inhomogeneous
distribution of PA in the two water and glycerol phases of the DNP juice (Weber et al., 2018). Such nanoscopic phase
separation were reported at a PA concentration of 10 – 80 mM, which could hamper the ¹H DNP efficiency by 20%.
The optimum ripening time (R_T) was reported to depend on the sample, polarizing agent and DNP juice composition.
Therefore, it is essential to investigate the impact of ripening time for diluted metabolite samples at natural ¹³C
180 abundance.

B. DNP Polarization

In this section, we describe the relevant instrumental details of the polarizer including the cryostat along with the
microwave source, followed by a discussion on the parameters involved in the optimization that impact repeatability
and sensitivity.

185 **DNP Polarizer:** The prototype Bruker d-DNP Polarizer works at field (7.05 T) and temperature (1.15 K) which offers
optimal CP based capabilities to reach high ¹³C polarization levels in about 15 minutes (Bornet et al., 2013; Dey et al.,
2020). It is built on a standard 7.05 T wide-bore magnet and cryostat design, modified to accommodate a variable
temperature insert (VTI). The VTI enables DNP at 1.15 K, using liquid helium (*l*-He) introduced from a transport
dewar (e.g., 100 L) and custom transfer line into a phase separator (PS) near the top of the VTI. From there, a membrane
190 pump (Vacuubrand MD 4 NT) transfers cold gaseous helium (*g*-He), whose enthalpy cools the neck, baffles & radiation
shields of the VTI, while *l*-He flows down from the PS and enters the sample space via automated needle valves near
the VTI tail. A main pump (Edwards iGx600L) acts on the admitted *l*-He for final cooling of the sample space, whose
temperature setpoint is chosen via feedback-controlled butterfly valve to the pump. For DNP, the microwave source

195 consists of a synthesiser (8-20 GHz), and an amplifier and frequency multiplier chain (AMC, Virginia Diodes, Inc) to deliver a final frequency of ~198 GHz at ~120 mW. A waveguide carries the μw into the VTI to irradiate the sample. Frequency modulation (Bornet et al., 2014) is programmed via the low-frequency source, while microwave gating (Bornet et al., 2016b) is achieved via TTL pulses from the Bruker AV NEO NMR console to the AMC. For NMR, the 2-channel console runs Topspin 4 and is coupled to a custom Bruker $^1\text{H},^{13}\text{C}$ probe, with an external tuning and matching (room temperature) for an overall circuit able to achieve simultaneous nutation frequencies of 50 kHz without arcing.

200 **Optimization:** The efficiency of the DNP polarization depends on the instrumental design (μw source, cryostat, polarizer, RF coil...). Therefore, the ability of users to improve sensitivity and repeatability is limited. Our system was designed to offer a highly repeatable polarization in the solid state, and further instrumental modifications are beyond the scope of this study. However, the sensitivity and repeatability are also impacted by user-dependent parameters, such as the polarization temperature, and the μw and CP parameters, which are further described below.

205 **B.1 Microwave parameters**

It is essential to find out the optimal μw irradiation frequency, power as well as associated modulation bandwidth to achieve optimal polarization. Optimal value of such parameters depends on the temperature and sample formulation. Here, μw optimization was performed at 1.2 K and for the optimal sample preparation parameters.

B.2 ^1H DNP build up

210 The measurement of ^1H polarization build-up rate helps to verify the PA's integrity and also dictates the optimum μw irradiation time (which is chosen to be once or twice the ^1H DNP build up time) between "contact" for polarization transfer from ^1H to ^{13}C via CP. For each sample, before polarizing the ^{13}C spins, the ^1H polarization build up time was measured using the pulse sequence shown in Figure B1a [at](#) 1.2K.

B.4 Vitrification parameters

215 Formation of a glass during vitrification inside the polarizer is important to obtain repeatable polarization. Care should be taken while inserting the sample to maintain a similar rate of vitrification in the cryostat. It is important to note that in some cases we experienced a sudden drop of ^1H polarization build-up time in spite of an identical sample composition, which resulted in a reduction of ^1H and ^{13}C DNP signal integrals. This could be due to the impact of the sample insertion rate on the formation of glassy matrix at cryo-temperature inside the cryostat. However, such reduction did not impact the liquid-state signal integral, [and we concluded that the vitrification rate did not impact our results](#). Still, to limit [potential associated such](#) effects, we took care of keeping the same sample insertion time (40 s) inside the cryostat for all experiments. Also, dissolving the metabolites and PA in H_2O and D_2O followed by dissolving the resulting solution in glycerol helped to improve the solid-state signal repeatability compared to the reverse sequence of dissolving the metabolites and PA in DNP juice (first in glycerol then in H_2O and D_2O).

225

B.3 CP parameters

As discussed in the introduction, achieving ^{13}C hyperpolarization via cross polarization (CP) from DNP polarized ^1H spins is the key for metabolomics application. The pulse sequence implemented to polarize ^{13}C nuclei is presented in Figure B1b. The optimization of CP parameters and the methodological developments ensuring efficient CP have been described thoroughly in previous studies (Elliott et al., 2021). Here, we followed a similar procedure of optimization and implemented these developments for our study.

C. Dissolution

After the completion of ^{13}C hyperpolarization at 1.2 K, the hyperpolarized sample is rapidly dissolved in a hot pressurized solvent, followed by a rapid transfer to the liquid-state spectrometer through a magnetic tunnel to minimize polarization losses due to the nuclear spin relaxation at room temperature during transfer. There are a number of developments aimed for rapid and robust dissolution process such as development of gas driven, liquid driven sample transfer systems (Katsikis et al., 2015; Ceillier et al., 2021; Bowen and Hilty, 2010), built-in sample transfer system attached to cold sample cup (Kress et al., 2021), solid sample transfer (Kouřil et al., 2019) etc. Each of the methods have their own advantages and disadvantages which have been reviewed in detail (Elliott et al., 2021). Here, we focus on the optimization of the gas driven dissolution system available on our setup.

In our case, dissolution is achieved upon manual coupling of a fluid transfer stick to the sample cup after it has been lifted (~9 cm) just above the l -He level. The stick includes two parallel capillaries (ETFE; 1.6 mm ID): an inlet for the preheated, ~~pressured~~-pressurized dissolution solvent and an outlet to carry hyperpolarized fluid via a sample transfer line to a 5 mm NMR tube situated in the probe of the solution-state NMR observation magnet. The hyperpolarized solid sample is dissolved in 5 ml of hot solvent and the helium gas drives the dissolved liquid inside the transfer line to run through a 0.56 T magnetic tunnel (Milani et al., 2015) (DNP Instrumentation, <https://dnp-instrumentation.com>). Inside the liquid-state NMR spectrometer, a passive receiver system (injector) accepts the turbulent dissolution sample, then facilitates phase separation (liquid sample and helium gas) and settling through gravity after introduction of the sample into the NMR tube at ambient temperature and pressure.

In this section, we discuss the experimental parameters related to the optimization of the dissolution, transfer and relax steps. In our previous study, the long duration of this process (time from the start of the dissolution to the start of the signal acquisition = 11.3 s) significantly reduced the sensitivity of ^{13}C metabolite signals (Dey et al., 2020). Moreover, the dissolution step contributes most to the signal unrepeatability as it involves a manual step. Therefore, careful optimization of the dissolution is crucial to ensure the maximum and repeatable amount of hyperpolarization before signal acquisition. From a technical point of view, the dissolution process consists of three main events: i) flushing the pre-pressurized hot solvent to the sample cup for certain duration (termed as “flush”, driven by the pressure difference between the pressure cooker and the sample space), ii) pushing (using Helium gas) the dissolved hyperpolarized sample for a fixed period of time (termed as “boost”) through the sample transfer line to reach to the injector, iii) collecting the liquid and allowing to release the pushing Helium gas (termed as “relax” duration) before reaching the dissolved sample to connected NMR tube. The “relax” time ensures to fill the liquid at least up to the active rf coil length devoid

of any microbubble, and to limit the residual motion of liquid that would impact the line shapes. A longer delay has a favourable impact in the improvement of signal line shape and linewidth, however resulting in sensitivity losses due to the polarization decay which impacts differently depending on the relaxation of different ^{13}C sites. The optimum value of the delay needs to be decided upon balancing the two opposing effects mentioned above to obtain better ^{13}C signal sensitivity for the majority of metabolites. Also, this delay depends on the physical properties (viscosity, surface tension etc.) of each dissolution solvent. Note that the relax delays contain a fixed duration delay (0.1 s trigger) of 0.1 which is required to switch/trigger the automatic signal acquisition pulse sequence in liquid-state spectrometer.

The scheme indicating three different stages of dissolution process is shown with different colour in Figure 1. There are several parameters involved in these three events which can be optimized to reduce the loss of polarization. We focused on the optimization of the following parameters:

C.1 Dissolution solvent (choice of solvent, solvent volume, dissolution pressure, dissolution temperature)

C.2 Dissolution duration (duration of flushing, boosting and relaxing)

C.3 Sample transfer line (length and inner diameter)

It is important to note that each all parameters listed above are correlated to each other. Therefore, we have focused on optimizing the combination of parameters instead of optimizing parameters one by one. Before presenting our attempts to find the best combination of parameters we introduce the influence of these parameters in the context of maximizing the available hyperpolarization in the liquid-state.

C.1 Dissolution solvent

The dissolution solvent has a significant impact on the efficiency of dissolving the hyperpolarized solid at a 1.2 K temperature, on the speed of sample transfer as well as on stabilizing the dissolved liquid inside NMR tube. D_2O is widely accepted as a dissolution solvent due to its high heat transfer coefficient, which leads to efficient dissolution of the hyperpolarized solid sample. Also, higher solubility of metabolites or other biological samples in D_2O forms an extra advantage. However, owing to its higher viscosity and surface tension, D_2O is less efficient in terms of sample transfer speed, and a longer stabilization delay is required to avoid microbubble during signal acquisition. Methanol- d_4 has been known to be used as an alternative dissolution solvent to boost the sample transfer rate and to reduce the stabilization delay as it is less viscous and has lower surface tension compared to D_2O (Singh et al., 2021b; Mishkovsky and Frydman, 2008). Both dissolution solvents have their own advantages and disadvantages. For example, the potential solubility of metabolites depends on the heat transfer efficiency, which in turn depends on the specific heat capacity and on the solvent temperature set at the dissolution box. Such specific heat capacity could be smaller for methanol- d_4 compared to D_2O (the specific heat capacity of water and methanol is about 4.18 kJ/kg K and 2.53 kJ/kg K respectively; for CD_3OD and D_2O we set the temperature in the dissolution oven at 156 °C and 170 °C respectively).

We decided to determine the best combination of dissolution parameters for both solvents. Note that the choice of solvent is limited to these two options owing to the incompatibility of the sample transfer material and the bad solubility of metabolites in other solvents.

The dissolution solvent volume influences the overall signal sensitivity in the liquid-state. Reducing the solvent volume decreases the dilution factor, which may either increase or decrease of signal sensitivity depending on the relative

influence of two opposing effects originating from the higher radical concentration in the dissolved sample vs. increase of sample spin concentration. However, a sufficient amount of dissolution solvent is necessary to efficiently dissolve the hyperpolarized solid inside the polarizer at a temperature of ~1 K. In our system, the dissolution solvent volume (5 mL) was already optimized by the instrument provider.

Dissolution temperature and pressure also play a role in efficiently dissolving and transferring the dissolved liquid. The choice of temperature is limited by the boiling point of the solvent at a particular pressure. Also, the choice of pressure is limited by the integrity of dissolution components. Therefore, these two parameters will be fixed as initial setting considered as a “safe” maximum value for our dissolution setup.

C.2 Dissolution duration

The optimum combination of “flush”, “boost” and “relax” durations is essential to reduce the overall dissolution time. The flush duration mainly impacts the sample melting process, the boost duration is responsible for transferring the dissolved sample through the sample transfer line and the relax duration is required to release the propellant helium gas avoiding microbubbles in the liquid-state sample before signal acquisition. Among all three durations, the boost and relax duration have the highest impact on fast sample transfer and improved signal line shape respectively. Therefore, optimization of the boost time and relax time is of highest priority in the optimization.

C.3 Sample transfer line

The inner diameter (ID) and length of sample transfer line influences the speed of sample transfer from the polarizer to the signal acquisition spectrometer and also, influences the formation of bubbles in the dissolved sample. In our present set up, two different ID (1.575 mm and 2.375 mm) of sample transfer line were available. We investigated the effect of ID of sample transfer line on the liquid-state signal sensitivity.

D. Signal acquisition

Upon completion of the dissolution process, the liquid sample is collected to the NMR tube by gravity and the pulse sequence automatically triggers to start signal acquisition, after a relax delay (discussed above). All d-DNP enhanced NMR experiments were recorded at room temperature on a 400 MHz Bruker Avance Neo spectrometer equipped with a liquid-N₂ cryogenically cooled probe (5 mm CryoProbe™ Prodigy BBFO with ATMA and Z-gradient from Bruker BioSpin) using standard optimized pulse sequence and calibrated pulse parameters. The ¹³C spectra were recorded in a single scan at a 90° flip angle using Waltz-16 ¹H decoupling during acquisition. They were processed with 1 Hz Lorentzian line-broadening, zero filled to 256 k data points, Fourier transformed, manually phase corrected and automatically baseline corrected with a polynomial of degree 5.

D.1 Pre-shimming and pre-tuning

Due to the rapidly decaying and irreversible nature of hyperpolarization, the method does not allow to perform tuning and shimming before acquisition of the signal on the hyperpolarized liquid sample. Therefore, the hyperpolarized

330 signal is acquired on pre-tuned and pre-shimmed condition. Pre-tuning and pre-shimming are done using similar
sample composition and maintaining similar sample height in the NMR tube as in the case of hyperpolarized signal
acquisition. Moreover, to achieved improved line shape it is desirable to perform pre-shimming at the similar
temperature as the temperature of hyperpolarized, dissolved liquid during signal acquisition. Note that to optimize the
quality of experiments in methanol, we have acquired a ^1H spectrum of the residual protonated methanol using the
335 the same dissolution settings with methanol- d_4 , and calculated the temperature of hyperpolarized liquid after injection (292
K) from the ^1H chemical shift difference of the methyl and -OH groups. Then, the pre-shimming of identical sample
was done at 292 K which helps to improve the line shape of ^{13}C signals. We noticed that DNP signal acquisition at 292
K improves linewidth of ^{13}C signals of metabolites by more than 11% compared to the DNP signal acquired at 298 K.

4. Results and Discussion

340 In this section, we describe the result of parameter optimization under each subunit in the experimental sequence of
events (sample preparation, polarization, dissolution, acquisition). In this section, each parameter is mentioned using
the numbering defined in Table 1. [Also, while comparing liquid state signals at different parameters optimization
stages, we analyzed only those signals which are above the limit of quantification \(SNR > 10\).](#) Figure 2 shows d-DNP
enhanced ^{13}C spectra of the metabolite mixture along with the reference, before experimental optimization of
345 parameters as used in the previous report (Dey et al., 2020). Note that apart for TSP which is more concentrated, only
quaternary carbons are visible due to their low signal to noise ratio (SNR).

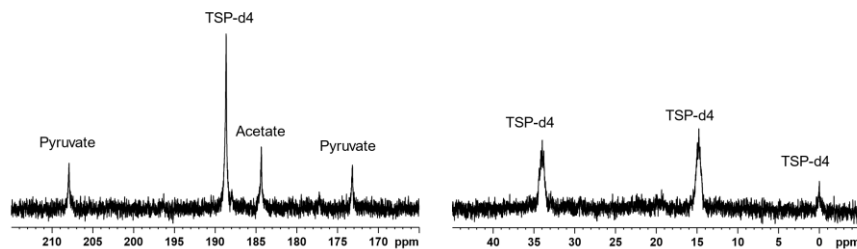


Figure 2. d-DNP enhanced ^{13}C - $\{^1\text{H}\}$ spectra of metabolites acquired before the optimization indicating all the relevant signals above the limit of detection.

350 A. Sample preparation

A.1 PA concentration

We compared three potentially suitable concentrations of TEMPOL (i.e. 75 mM, 50 mM, 25 mM). The ^1H DNP polarization build up time for 75 mM, 50 mM, 25 mM of TEMPOL were 20 s, 53 s, > 3600 s respectively (Figure C1). Here, to maintain high throughput conditions, we compared the DNP polarization of ^{13}C at different TEMPOL
355 concentration with a fixed ^{13}C DNP polarization time of about 20 mins (using contact time of 15 ms which was found

to be optimal for each radical concentration and 80 s of μw irradiation per each cycle of polarization transfer $^1\text{H} \rightarrow ^{13}\text{C}$ (CP contact)). Figure 3 compares DNP-enhanced ^1H and ^{13}C signal in the solid-state, as well as liquid-state ^{13}C signal integrals at same polarization duration. Note that the differences of signal integral at different radical concentration do not quantitatively reflect the polarization due to bleaching effect in solid state (Stern et al., 2021). Nevertheless, at a 50 mM radical concentration, the solid-state as well as liquid-state signals are particularly more sensitive than other TEMPOL concentration at a fixed experimental time. It is important to note that although the protonated carbon of TSP shows slightly higher sensitivity at 25 mM TEMPOL due to smaller relaxation losses during dissolution, however, the sensitivity of other ^{13}C signals is considerably lower compared to 50 mM TEMPOL. At 25 mM TEMPOL, it would be possible to achieve similar DNP polarization as at 50 mM TEMPOL but at the cost of an order of magnitude higher experimental time.

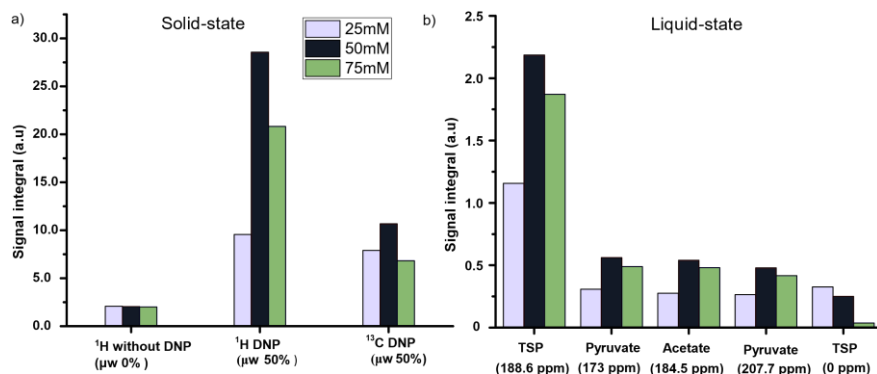


Figure 3. Comparison of signal integral value of a) ^1H and ^{13}C signals in the solid-state and b) ^{13}C - $\{^1\text{H}\}$ liquid-state signal integrals of metabolites with a 25 mM, 50 mM and 75 mM TEMPOL concentration.

A.2 “DNP juice” composition

We have investigated the DNP efficiency of two different compositions of DNP juice (5:4:1 and 6:3:1 Glycerol- d_8 : D₂O: H₂O, v/v), which have been reported to be efficient conditions for polarization with nitroxide based radicals. As noted in the previous section, further increase in glycerol content would result in an insolubility of metabolites in the DNP juice. It is worthwhile to note that in our previous DNP based metabolomic work, the composition of the DNP juice was 5:4:1. Figure 4a compares the ^1H and ^{13}C signal integral values at two different DNP juice composition, which shows that DNP juice composition of 6:3:1 (Glycerol- d_8 : D₂O: H₂O, v/v) offers higher polarization compared to the 5:4:1 (Glycerol- d_8 : D₂O: H₂O, v/v) with similar repeatability. Further increase in glycerol content could reduce the solubility of metabolites which may hinder the metabolomic application in general. Therefore, the optimized DNP juice composition will be 6:3:1 for the rest of the study.

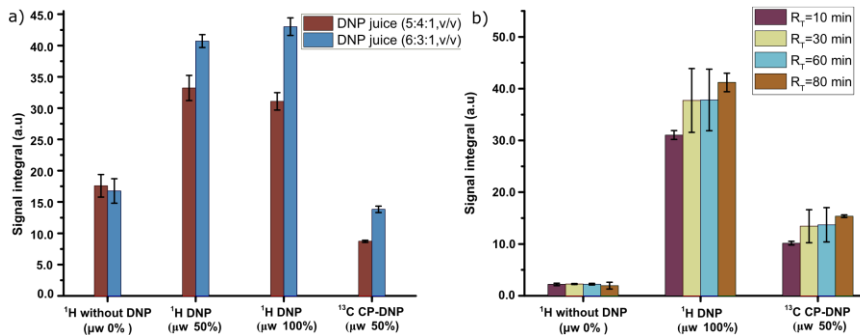


Figure 4. a) Plot of solid-state ¹H thermal-signal without μw as well as ¹H and ¹³C DNP signal integrals at two different DNP juice compositions with 50 mM TEMPOL using optimized μw parameters; b) Plot of solid-state ¹H and ¹³C thermal-signal without μw as well as DNP signal integral at different ripening time with same TEMPOL concentration using optimized μw parameters. The standard deviation for every average integral value is calculated from 3 identical samples and displayed as an error bar.

Mis en forme : Police :Symbol

380

385 A.3 Ripening time

With our sample of choice and DNP juice, we did not find any considerable change of polarization after 30 mins of ripening time (defined as the sum of time elapsed from sample preparation to insertion in the freezer and from the freezer to insertion inside the polarizer) as reflected in figure 4b. Therefore, we chose to systematically wait 30 mins at room temperature before vitrifying the sample inside the DNP polarizer, and also to prepare all the samples at the same room temperature to avoid unnecessary sources of signal variation.

390

B. DNP Polarization

B.1 Microwave optimization

In Figure A1, we show the evolution of the relative ¹H signal integral vs μw frequency and power. From this plot, we have chosen 198.08 GHz as an optimized frequency which corresponds to the negative DNP polarization and 50% of available μw power for CP based ¹³C polarization. We also investigated the effect of the μw modulation bandwidth for efficient μw excitation by observing the ¹H signal integral at different modulation bandwidths and frequencies. The optimum values (a triangular frequency modulation with at bandwidth (Δf_{μw}) of ± 5 MHz and frequency of 10 kHz is used) remained unchanged from our previously reported studies.

395

B.2 ¹H DNP build-up

We measured the ¹H build up time of our sample at a 50 mM TEMPOL concentration with optimum DNP juice composition at 1.2 K, leading to an estimated value of 53 s with 5% variation over successive experiments.

400


B.3 CP parameters

405 After optimization, the ^1H polarization is transferred to ^{13}C by 16 CP contacts of 15 ms each at intervals of 80 s, with a radiofrequency (RF) power of 15 W on ^1H (using rectangular pulse with constant RF amplitudes of 21 kHz) and 60 W on ^{13}C (using ramped up pulse with linearly increasing RF amplitudes from 16 kHz to 23.2 kHz). Adiabatic half passage pulses (WURST) of 30 W and 60 W (pulse duration of 175 μs , sweep width of 100 kHz) were used on ^1H and ^{13}C channels respectively before and after the CP contacts. The total duration of CP experiment was 21 min.

C. Dissolution

410 C.2 Dissolution timing optimization

Before optimization, the duration of “flush”, “boost” and “relax” times were set to 0.2 s, 5 s, 6.1 s. We have considered this total duration of dissolution time (flush, boost and relax, 11.3 s) as an upper limit with the objective to reduce the duration in the optimization process. Among the three durations, the boost time is the most critical duration for optimization. Therefore, we first focused on comparing several “boost” durations by analyzing the ^{13}C signal of metabolites with a fixed set of flush time (0.2 s) and relax time (2.1 s). The results presented in Figure 5 were obtained 415 using a capillary transfer line with 1.575 mm inner diameter and a length of 370 cm with D_2O as a dissolution solvent.

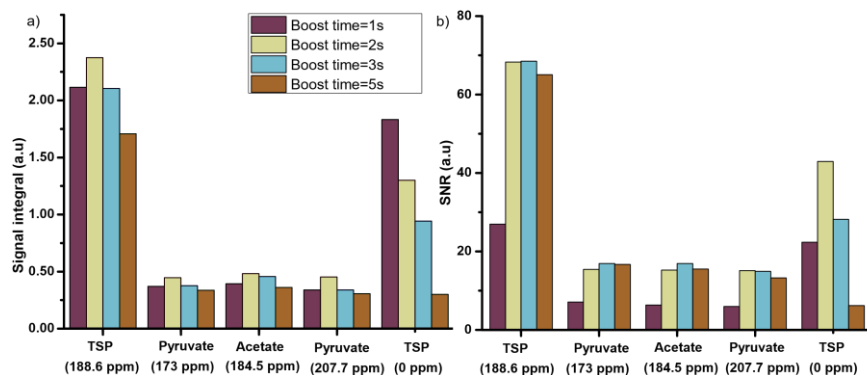

420 Figure 5. Plot of liquid-state hyperpolarized ^{13}C - $\{^1\text{H}\}$ signal integrals (a) and SNR (b) of the metabolites at different boost times using optimized μw and solid-state DNP parameters using a transfer line with 1.575 mm ID and D_2O as dissolution solvent. The optimum value of boost time is chosen to be 2 s.

The comparison shows improved signal integral values as the boost time is reduced from 5 s to 1 s. Due to the reduction of boost time, the fast-relaxing protonated ^{13}C signal (the protonated ^{13}C signal of TSP at 0 ppm) shows significant improvement compared to the quaternary ^{13}C , but protonated ^{13}C signals from other metabolites remain invisible. However, SNR comparison in Figure 5 (b) indicates an optimum boost time of 2 s corresponding to an improved line shape. Similar comparison with methanol- d_4 solvent exhibit the same boost time duration of 2 s for optimal sample 425 transfer.

We have compared the repeatability of the newly optimized boost time with the repeatability before optimization (Figure 6). Figure 6 shows improved signal integral (especially for the protonated ^{13}C of TSP) while retaining similar repeatability at the optimized dissolution duration. Following the optimization of the boost time, we also tested different flush times (data not shown) at a fixed boost duration and relax duration of 2 s and 1.1 s respectively. Overall, it was found that the reduction of flush durations did not improve signal sensitivity for both dissolution solvents.

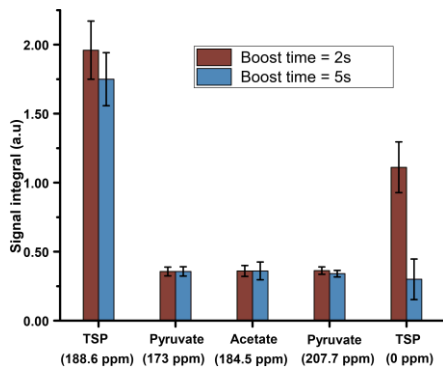



Figure 6. Plot of liquid-state hyperpolarized ^{13}C - $\{^1\text{H}\}$ signal integral repeatability before and after optimized dissolution timings using 1.575 mm ID of transfer line and D_2O as dissolution solvent keeping flush and relax delay of 2.1 s.

As mentioned earlier in the experimental section, the relax time optimization is crucial to have an improved spectral line shape of hyperpolarized ^{13}C signal with minimum loss of polarization. In the following section, we show the relax time optimization result at a fixed flush duration and boost duration of 0.2 s and 2 s, respectively, for the two dissolution solvents (methanol- d_4 , D_2O) separately as this optimization is solvent specific.

C.1 Dissolution solvent

With D_2O as dissolution solvent, the protonated and the quaternary ^{13}C signal of TSP at 2.1 s of relax time offers significant improvement of sensitivity compared to other relax values (see Figure 7a). Here, considering a significant sensitivity improvement ^{13}C signals, we set 2.1 s as an optimum relax time *with the cost of slightly lower sensitivity compared to other relax time*. With CD_3OD , we obtained optimum sensitivity at 1.1 s of relax time despite the irregular behavior of the quaternary ^{13}C of alanine at 4.1 s and protonated ^{13}C of TSP (see Figure 7b). Indeed, with CD_3OD , the dissolved sample stabilizes more quickly compared to D_2O owing to the lower viscosity and surface tension of CD_3OD . Although, at relax time = 1.1 s we obtained optimum SNR with CD_3OD , we experienced some random failures in signal acquisition. Systematic investigation of this failure revealed that caution needs to be taken at the connection point of injector and NMR tube to avoid failure in acquiring signal at 1.1 s of relax time.

Mis en forme : Exosant

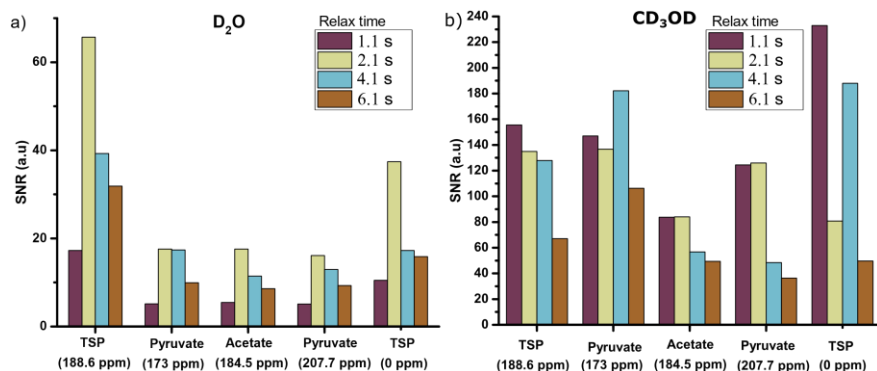

450 Figure 7: Sensitivity comparison of $^{13}\text{C}\{-^1\text{H}\}$ signal at different relax time using a) D_2O and b) CD_3OD as dissolution solvent. The optimum relax time with D_2O and CD_3OD are chosen to be 2.1 s and 1.1 s.

As indicated in figure E1, the NMR tube should be exactly connected to the bottom end of the injector as the imperfect connection at the junction between the injector and NMR tube causes inefficient filling of liquid in the NMR tube before the start of signal acquisition. This often results in ~~to~~ failure ~~in~~ of signal acquisition. We have designed a special gauge to ensure proper positioning of the NMR tube in the injector, which completely solved such failure issue. In a nutshell, the optimum total duration of the dissolution time (time from the start of the dissolution to the start of the signal acquisition) was set to 4.3 s and 3.3 s considering flush, boost and relax durations of 0.2 s, 2 s, 2.1 s for D_2O and 0.2 s, 2 s, 1.1 s for CD_3OD respectively. To appreciate the impact of dissolution time optimization we have measured the T_1 values of metabolites in the presence (at final concentration of TEMPOL after dissolution) and absence of TEMPOL as presented in Table 2.

460 Table 2. T_1 values of metabolites in D_2O in the presence and absence of TEMPOL.

| Metabolites | Relaxation Time (T_1 , s) | |
|---|------------------------------|----------------|
| | With TEMPOL | Without TEMPOL |
| <u>Pyruvate (207.7 ppm)</u> | <u>13.6</u> | <u>22.8</u> |
| <u>TSP-d_4 (188.6 ppm)</u> | <u>6.1</u> | <u>35.2</u> |
| <u>Acetate (184.4 ppm)</u> | <u>12.4</u> | <u>51.8</u> |
| <u>Alanine (177.2 ppm)</u> | <u>12.3</u> | <u>28.2</u> |
| <u>Pyruvate (172.6 ppm)</u> | <u>14.3</u> | <u>41.0</u> |
| <u>Acetate (26 ppm)</u> | <u>6.2</u> | <u>10.4</u> |
| <u>Pyruvate (28.9 ppm)</u> | <u>6.4</u> | <u>11.7</u> |
| <u>TSP-d_4 (0 ppm)</u> | <u>3.0</u> | <u>5.2</u> |

← **Tableau mis en forme**

← **Mis en forme** : Espace Avant : Automatique, Après : 6 pt, Interligne : simple

← **Mis en forme** : Espace Avant : Automatique, Après : 6 pt, Interligne : simple

These T_1 measurements were done by dissolving the metabolites (each at 500 mM concentration) in D_2O with similar composition of DNP juice present in the post-dissolution solution. -Table 2 helps to evaluate the role of longitudinal

475 relaxation in the effect of the optimization of the dissolution time on the observed hyperpolarization in solution. Similar
 T_1 measurements in CD_3OD could not be performed as metabolites at a 500 mM concentration and even at a 100 mM
concentration (particularly alanine and pyruvate) were not soluble enough in CD_3OD . However, relative differences
in T_1 relaxation values may be anticipated to follow similar trends as in D_2O . Overall, CD_3OD as a dissolution solvent
compared to D_2O showcases superior performance by offering better lineshape which translates into improved signal
sensitivity of our model metabolite mixture sample. However, for the wide range of biological samples, lack of
chemical shift database of metabolites and inefficient solubility of metabolites in CD_3OD could impose additional
480 challenges. On the one hand, the chemical shift assignment challenge in CD_3OD could be overcome by “spiking”
experiments. On the other hand, previous studies showed that aqueous solvent based dissolution techniques can be
improved by using back-pressure techniques(Kouřil et al., 2021, 2019; Katsikis et al., 2015; Bowen and Hilty, 2010;
Ceillier et al., 2021). Therefore, in general, the choice the dissolution solvent between CD_3OD and D_2O should be
weighed by considering such factors.


485 C.3 Transfer line optimization

First, we suitably adjusted the length (370 cm) of sample transfer line according to the distance between polarizer and NMR acquisition magnet by reducing the extra length of the line that was present in the initial setting. The effect of the transfer line inner diameter on the signal integral values along with the repeatability is presented in Figure D1, which shows superior signal obtained with the small diameter ID (1.575 mm) transfer line compared to the wider one (2.375 mm). A possible explanation for such difference in the signal integral would be better homogeneity and smaller segregation of the liquid and gas mixture in the smaller ID of sample transfer line compared to the wider ID resulting in a faster sample mass transfer. To maintain signal line shape repeatability, care should be taken at the connection point of sample transfer line to the dissolution stick and injector.

5. Result of optimization

495 Finally, we have compared the metabolite signal integrals and sensitivity to investigate the performance of the two dissolution solvents with the optimized d-DNP setting and benchmarked the improvement of signal with respect to the spectrum acquired before optimization of d-DNP settings (see spectra in Figure 8). Figure 9 showcases significant improvement in sensitivity (about 5 times improvement on quaternary ^{13}C and 50 times improvement on protonated ^{13}C) as well as improvement in signal integral especially with CD_3OD compared to signals obtained using the initial parameters before DNP optimization. The main contributing factors of this improvement are the shorter dissolution duration and faster stabilization of the dissolved liquid inside the NMR tube. These factors also contributed to improve the line shape and the linewidth of ^{13}C signals with CD_3OD (see spectra in Figure 8) significantly (at least 3 times sharper). We found that after optimization the improved sensitivity with CD_3OD enables the detection and analysis of
the quaternary alanine signal which was not detected before. Moreover, the overall optimization improved the limit of
505 detection which enabled the observation of the protonated ^{13}C signals of metabolites at natural abundance (e. g. signals
of acetate and pyruvate at 29 ppm and 26 ppm).

Mis en forme : Indice

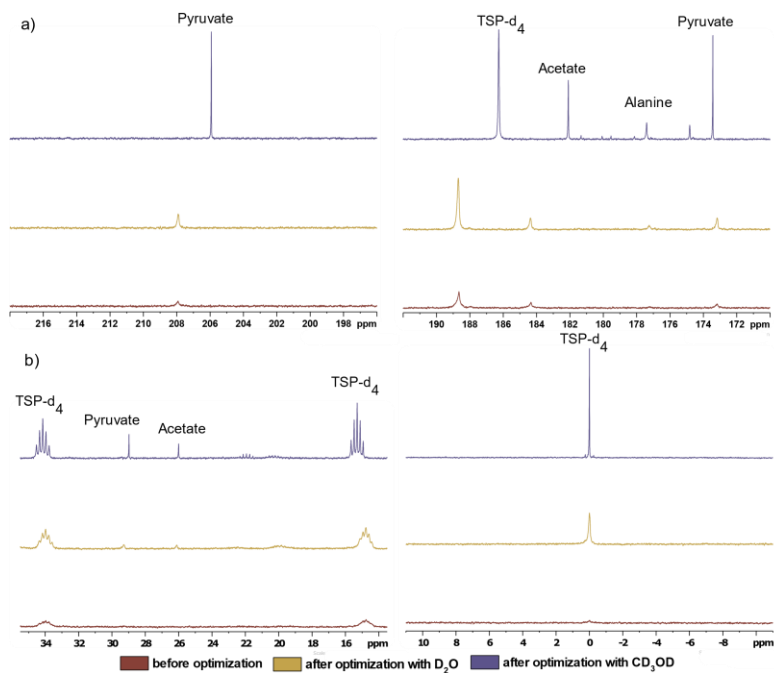

510 Figure 8. Comparison of $^{13}\text{C}\{-^1\text{H}\}$ spectra of metabolites before and after optimization in the a) quaternary ^{13}C region and b) protonated ^{13}C region using two dissolution solvents.

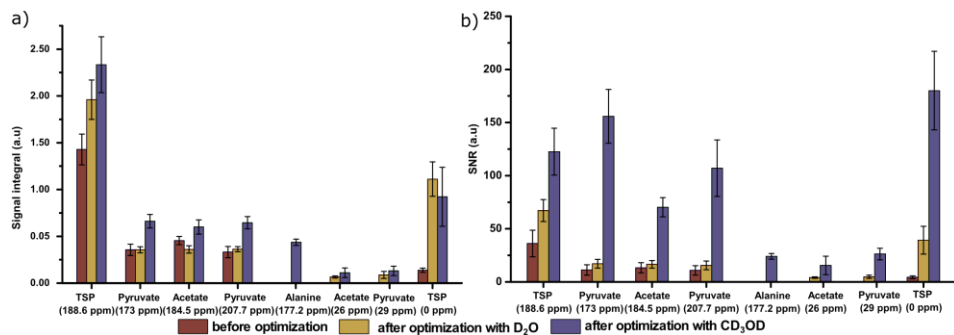


Figure 9. Comparison of $^{13}\text{C}\{-^1\text{H}\}$ signals of metabolites with respect to a) average signal integral and b) average sensitivity along with the standard deviation, with and without systematically optimized parameters using two dissolution solvents.

515

We have summarized the impact of optimization in Table 3 which showcases the changes in spectral qualities of signals (signal integral repeatability, linewidth, liquid state polarization) before and after optimization of the d-DNP setting. Table 3 highlights the significant improvement of the linewidth and liquid state polarization (specially with CD₃OD).

Table 23. Repeatability comparison of ¹³C-¹H signal integral of metabolites with and without systematically optimized parameters, and with two different dissolution solvents.

| Metabolites | Experimental Condition | Repeatability (cv %) | | Linewidth (Hz) | Liquid state Polarization ^c (%) |
|-----------------------------------|----------------------------|----------------------|----------------|----------------|--|
| | | Absolute | Normalized | | |
| Pyruvate (207.7 ppm) | Before | 18.2 | 6.6 | 11.6 | 8.0 |
| | After (D ₂ O) | 7.4 | 6.5 | 8.3 | 8.0 |
| | After (CD ₃ OD) | 10.1 | 3.0 | 1.8 | 15.0 |
| TSP-d ₄ (188.6 ppm) | Before | 11.5 | ^a | 13.0 | 9.0 |
| | After (D ₂ O) | 10.7 | - ^a | 9.1 | 14.0 |
| | After (CD ₃ OD) | 12.8 | - ^a | 6.6 | 17.0 |
| Acetate (184.4 ppm) | Before | 9.8 | 3.0 | 12.1 | 12.0 |
| | After (D ₂ O) | 10.9 | 3.9 | 8.7 | 11.0 |
| | After (CD ₃ OD) | 12.6 | 0.9 | 2.7 | 18.0 |
| Alanine (177.2 ppm) | Before | - ^b | - ^b | - ^b | - ^b |
| | After (D ₂ O) | - ^b | - ^b | 14.1 | 5.0 |
| | After (CD ₃ OD) | 8.0 | 5.5 | 6.7 | 9.0 |
| Pyruvate (172.6 ppm) | Before | 17.0 | 8.1 | 11.6 | 9.0 |
| | After (D ₂ O) | 9.0 | 6.2 | 8.4 | 11.0 |
| | After (CD ₃ OD) | 11.0 | 2.1 | 1.1 | 19.0 |
| Acetate (26 ppm) | Before | - ^b | - ^b | - ^b | - ^b |
| | After (D ₂ O) | 17.0 | 26.3 | 10.1 | 2.0 |
| | After (CD ₃ OD) | 46.0 | 51.0 | 2.7 | 4.0 |
| Pyruvate (28.9 ppm) | Before | - ^b | - ^b | - ^b | - ^b |
| | After (D ₂ O) | 43.0 | 50.0 | 8.2 | 3.0 |
| | After (CD ₃ OD) | 39.0 | 33.0 | 1.6 | 6.0 |
| TSP-d ₄ (0 ppm) | Before | 16.1 | 17.3 | 13.5 | 0.4 |
| | After (D ₂ O) | 16.5 | 8.0 | 8.3 | 2.0 |
| | After (CD ₃ OD) | 34.1 | 29.7 | 1.1 | 3.0 |

^a Normalized signal repeatability were obtained from the normalized signal integral with respect to TSP-d₄ (188.6 ppm).

^b Peak areas were not measured when the signals were below the limit of quantification (SNR<10).

^c Liquid state polarization was calculated by comparing the thermal signal integral at a 500 mM concentration of metabolites acquired with similar acquisition parameters as d-DNP and the polarization values are rounded off suitably.

In order to evaluate the impact of optimization on repeatability, Table 2-3 also compares the repeatability of absolute and normalized signal integrals (with respect to TSP signal at 188 ppm). The results demonstrate a considerable improvement for the quaternary ¹³C signals in both solvents after optimization compared to the signal obtained before

525

Mis en forme : Police :10 pt

Mis en forme : Police :10 pt

Mis en forme : Police :10 pt

Mis en forme : Police :10 pt

Mis en forme : Police :10 pt

Mis en forme : Police :9 pt, Exposit

Mis en forme : Police :9 pt, Exposit

Mis en forme : Police :9 pt, Exposit

Mis en forme : Police :9 pt, Exposit

Mis en forme : Police :9 pt

Mis en forme : Police :9 pt, Non Exposit/ Indice

Mis en forme : Police :9 pt

Mis en forme : Police :9 pt

Mis en forme : Police :9 pt, Indice

Mis en forme : Police :9 pt

Mis en forme : Police :9 pt

Mis en forme : Police :9 pt

Mis en forme : Police :9 pt

Mis en forme : Exposit

Mis en forme : Non Exposit/ Indice

Mis en forme : Police :9 pt

Mis en forme : Police :9 pt

Mis en forme : Police :9 pt

Mis en forme : Police :9 pt, Exposit

530 optimization. However, reduction of the dissolution time and stabilization delay introduces additional challenges in the manual dissolution efficiency to maintain the repeatability of the protonated ^{13}C as the T_1 relaxation value of the fast-relaxing protonated ^{13}C spins in presence of 2 mM TEMPOL (final concentration of radical after dissolution) is about 5–6 s. We found that the TSP signal at 0 ppm and the protonated ^{13}C signals of metabolites showed much higher variability. The T_1 value (Table 2) of protonated TSP is the minimum among all the peaks of our interest which can be linked to the much higher associated signal variability. In future DNP enhanced metabolomics study, care should be taken when choosing the reference signals. T_1 measurements under DNP conditions could provide a hint towards the choice of a reference, as presented in table 2. The higher variability of the protonated ^{13}C signals of the metabolites may be linked to their lower sensitivity which occurs due to the combined effect of shorter relaxation times compared to TSP- d_4 . Future optimization study will focus on further improving the repeatability of protonated ^{13}C signal by better controlling the repeatability of dissolution step.

6. Conclusion


540 We have presented the detailed report of a fine, user-oriented optimization of a semi-automated, prototype d-DNP experimental setting dedicated to ^{13}C NMR of metabolite mixtures at natural abundance. The optimization allows to extend the scope of natural abundance ^{13}C metabolomics studies with high repeatability. The optimized conditions make it possible to identify the previously inaccessible protonated- ^{13}C signals of metabolites with improved line shape. Still, it also opens the way to further optimization. In the near future, with the present d-DNP setting it would be interesting to investigate the impact of a few parameters that would require minor modifications of the instrumental setting such as effect of magnetic tunnel, dissolution solvent volume, length and geometry of the injector etc. However,

545 ~~Further~~ improvement of the signal repeatability of ^{13}C signals (especially the protonated ^{13}C spins) will probably require more extensive instrumental developments such as automated dissolution system, rapid sample transfer module, etc. ~~In the future,~~ ~~The Further~~ reduction of the dissolution, transfer and stabilization delays could even enable the acquisition of DNP enhanced ^1H spectra of the metabolites. Also, recent report on the use of porous polarizing matrices could provide a tremendous boost for metabolomic applications as it makes DNP highly independent on the sample and it removes paramagnetic relaxation in the liquid-state. (Cavallès et al., 2018; El Daraï et al., 2021); Overall, we have established a series of optimization guidelines which could be of general interest for analytical applications of d-DNP NMR. We hope that such optimized d-DNP NMR setting will pave the way to new applications of hyperpolarized ^{13}C NMR of complex mixtures at natural abundance.

550

555


Appendix A: μ w frequency and power optimization

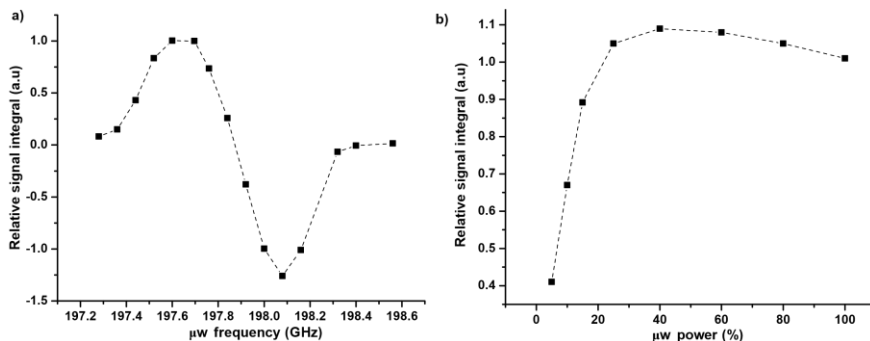

560 Figure A1. a) Plot of relative ^1H DNP signal integral vs. μ w frequency at 50 mM TEMPOL. Signals are normalized with respect to the signal at 197.69 GHz. b) Plot of relative ^1H DNP signal integral vs. μ w power (%). Signals are normalized with respect to the signal at 198.08 GHz with a triangular frequency modulation with a bandwidth ($\Delta f_{\mu w}$) of ± 5 MHz and frequency of 10 kHz.

Appendix B: Pulse programme to monitor ^1H DNP build-ups and solid-state DNP pulse sequence via cross polarization (CP)


565

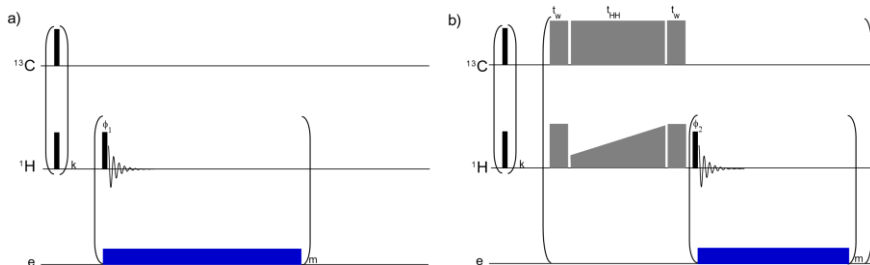

570 Figure B1. Pulse sequence used to monitor a) ^1H DNP build-ups and b) solid-state DNP pulse sequence via cross polarization (CP) for d-DNP. A train ($k=64$) of $\pi/2$ pulses was applied to both RF channels for pre-saturation. For ^1H build-up measurements, a small flip angle radiofrequency (RF) pulse is employed after each μ w irradiation of 10 s (depicted as "blue" block) to monitor the polarization level. Here CP (depicted as "grey" blocks) is performed using adiabatic half passage pulses ($t_w = 175 \mu\text{s}$) to convert longitudinal magnetization into transverse magnetization before the start of the contact pulse ($t_{\text{HH}} = 15 \text{ ms}$) and vice versa after the contact. Contact pulses use RF powers of 15 W on ^1H (using rectangular pulse with constant RF amplitudes of 21 kHz) and 60 W on ^{13}C (using ramped up pulse with linearly increasing RF amplitudes from 16 kHz to 23.2 kHz). In total, 16 CP contacts ($n=16$) are made. For each contact, a sequence of $m=4$ pulses with low-flip-angle pulse (5°) is applied on ^{13}C channel to monitor the build-up of the


polarization from ^1H to ^{13}C . Microwave irradiation is selectively switched on after each CP contact for 80 s to improve DNP polarization efficiency by avoiding the significant contribution of electron spin in nuclear spin relaxation rate

Appendix C: ^1H DNP polarization build up plot at different radical concentration

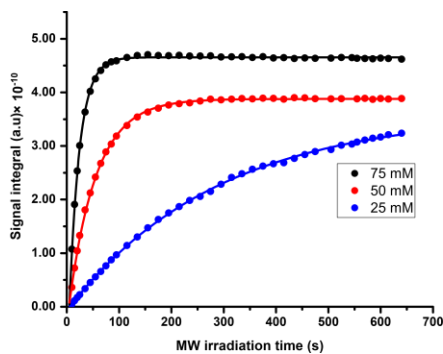


580 Figure C1. ^1H DNP polarization build up plot at different TEMPOL concentration (75 mM, 50 mM, 25 mM). The data points are fitted monoexponentially to obtain the DNP build-up rate.

Appendix D: Sample transfer line optimization

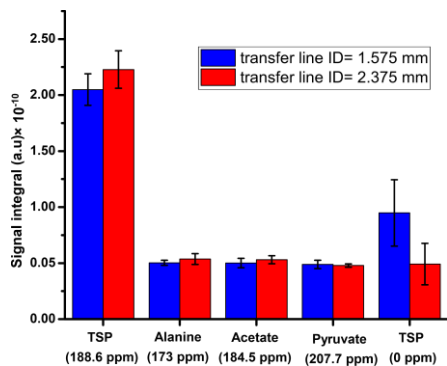

585 Figure D1. Comparative plot of liquid-state ^{13}C signal integral between two different sample transfer line inner diameters at same dissolution delay.

Appendix E: Injector and NMR tube connection

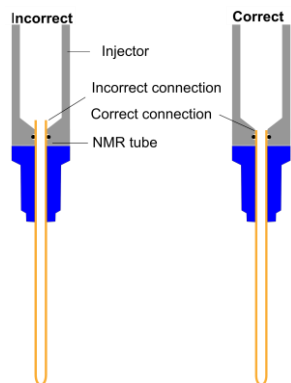

590

Figure E1: Schematic presentation of correct and incorrect connections between the top part of the NMR tube and injector.

Data availability

595 The NMR data shown in Figure 2 to figure 9 are available for download in TopSpin format from <https://doi.org/10.5281/zenodo.6810794>

Author contributions

All co-authors designed the experiments. AD, BC, KL and VR carried out the experiments and analyzed the data. AD, JND and PG prepared the manuscript with contributions from all co-authors.

Competing interests

600 The authors declare the following competing financial interest(s): D.E., M.S., R.M., and J.G.K. are employees of Bruker Biospin, which supplied the d-DNP polarizer. It is not a commercial instrument but a step in ongoing Bruker R&D.

Acknowledgements

605 This work has received funding from the European Research Council (ERC) under the European Union's Horizon 2020 research and innovation program (grant agreements no 801774/DINAMIX, 814747/SUMMIT, 714519/HP4all), Marie

Skłodowska-Curie grant agreement no. 766402/ZULF, the Region Pays de la Loire (Connect Talent) and ENS-Lyon, the French CNRS, Nantes Université, Lyon 1 University. The authors also acknowledge the French National Infrastructure for Metabolomics and Fluxomics MetaboHUB-ANR-11-INBS-0010 (www.metabohub.fr) and the Corsaire metabolomics core facility (Biogenouest). This work includes NMR experiments carried out on the CEISAM NMR platform.

References

- Ardenkjær-Larsen, J. H., Fridlund, B., Gram, A., Hansson, G., Hansson, L., Lerche, M. H., Servin, R., Thaning, M., and Golman, K.: Increase in signal-to-noise ratio of > 10,000 times in liquid-state NMR, *Proc. Natl. Acad. Sci. U.S.A.*, 100, 10158–10163, <https://doi.org/10.1073/pnas.1733835100>, 2003.
- 615 Batel, M., Däpp, A., Hunkeler, A., Meier, B. H., Kozerke, S., and Ernst, M.: Cross-polarization for dissolution dynamic nuclear polarization, *Phys. Chem. Chem. Phys.*, 16, 21407–21416, <https://doi.org/10.1039/C4CP02696A>, 2014.
- Bornet, A., Melzi, R., Perez Linde, A. J., Hautle, P., van den Brandt, B., Jannin, S., and Bodenhausen, G.: Boosting Dissolution Dynamic Nuclear Polarization by Cross Polarization, *J. Phys. Chem. Lett.*, 4, 111–114, <https://doi.org/10.1021/jz301781t>, 2013.
- 620 Bornet, A., Milani, J., Vuichoud, B., Perez Linde, A. J., Bodenhausen, G., and Jannin, S.: Microwave frequency modulation to enhance Dissolution Dynamic Nuclear Polarization, *Chemical Physics Letters*, 602, 63–67, <https://doi.org/10.1016/j.cplett.2014.04.013>, 2014.
- 625 Bornet, A., Maucourt, M., Deborde, C., Jacob, D., Milani, J., Vuichoud, B., Ji, X., Dumez, J.-N., Moing, A., Bodenhausen, G., Jannin, S., and Giraudeau, P.: Highly Repeatable Dissolution Dynamic Nuclear Polarization for Heteronuclear NMR Metabolomics, *Anal. Chem.*, 88, 6179–6183, <https://doi.org/10.1021/acs.analchem.6b01094>, 2016a.
- 630 Bornet, A., Pinon, A., Jhajharia, A., Baudin, M., Ji, X., Emsley, L., Bodenhausen, G., Ardenkjær-Larsen, J. H., and Jannin, S.: Microwave-gated dynamic nuclear polarization, *Phys. Chem. Chem. Phys.*, 18, 30530–30535, <https://doi.org/10.1039/C6CP05587G>, 2016b.
- Bowen, S. and Hilty, C.: Rapid sample injection for hyperpolarized NMR spectroscopy, *Phys. Chem. Chem. Phys.*, 12, 5766, <https://doi.org/10.1039/c002316g>, 2010.
- 635 Calvani, R., Miccheli, A., Capuani, G., Tomassini Miccheli, A., Puccetti, C., Delfini, M., Iaconelli, A., Nanni, G., and Mingrone, G.: Gut microbiome-derived metabolites characterize a peculiar obese urinary metabolite, *Int J Obes*, 34, 1095–1098, <https://doi.org/10.1038/ijo.2010.44>, 2010.
- Cavallès, M., Bornet, A., Jaurand, X., Vuichoud, B., Baudouin, D., Baudin, M., Veyre, L., Bodenhausen, G., Dumez, J.-N., Jannin, S., Copéret, C., and Thieuleux, C.: Tailored Microstructured Hyperpolarizing Matrices for Optimal Magnetic Resonance Imaging, *Angew. Chem.*, 130, 7575–7579, <https://doi.org/10.1002/ange.201801009>, 2018.
- 640 Ceillier, M., Cala, O., El Daraï, T., Cousin, S. F., Stern, Q., Guibert, S., Elliott, S. J., Bornet, A., Vuichoud, B., Milani, J., Pages, C., Eshchenko, D., Kempf, J. G., Jose, C., Lambert, S. A., and Jannin, S.: An automated system for fast transfer and injection of hyperpolarized solutions, *Journal of Magnetic Resonance Open*, 8–9, 100017, <https://doi.org/10.1016/j.jmro.2021.100017>, 2021.
- 645 Clendinen, C. S., Lee-McMullen, B., Williams, C. M., Stupp, G. S., Vandenborne, K., Hahn, D. A., Walter, G. A., and Edison, A. S.: ¹³C NMR Metabolomics: Applications at Natural Abundance, *Anal. Chem.*, 86, 9242–9250, <https://doi.org/10.1021/ac502346h>, 2014.

Mis en forme : Anglais (États-Unis)

- Daniele, V., Legrand, F.-X., Berthault, P., Dumez, J.-N., and Huber, G.: Single-Scan Multidimensional NMR Analysis of Mixtures at Sub-Millimolar Concentrations by using SABRE Hyperpolarization, *ChemPhysChem*, 16, 3413–3417, <https://doi.org/10.1002/cphc.201500535>, 2015.
- 650 Dey, A., Charrier, B., Martineau, E., Deborde, C., Gandriau, E., Moing, A., Jacob, D., Eshchenko, D., Schnell, M., Melzi, R., Kurzbach, D., Ceillier, M., Chappuis, Q., Cousin, S. F., Kempf, J. G., Jannin, S., Dumez, J.-N., and Giraudeau, P.: Hyperpolarized NMR Metabolomics at Natural ^{13}C Abundance, *Anal. Chem.*, 92, 14867–14871, <https://doi.org/10.1021/acs.analchem.0c03510>, 2020.
- 655 Dumez, J.-N., Milani, J., Vuichoud, B., Bornet, A., Lalande-Martin, J., Tea, I., Yon, M., Maucourt, M., Deborde, C., Moing, A., Frydman, L., Bodenhausen, G., Jannin, S., and Giraudeau, P.: Hyperpolarized NMR of plant and cancer cell extracts at natural abundance, *Analyst*, 140, 5860–5863, <https://doi.org/10.1039/C5AN01203A>, 2015.
- El Daraï, T. and Jannin, S.: Sample formulations for dissolution dynamic nuclear polarization, *Chem. Phys. Rev.*, 2, 041308, <https://doi.org/10.1063/5.0047899>, 2021.
- 660 El Daraï, T., Cousin, S. F., Stern, Q., Ceillier, M., Kempf, J., Eshchenko, D., Melzi, R., Schnell, M., Gremillard, L., Bornet, A., Milani, J., Vuichoud, B., Cala, O., Montarnal, D., and Jannin, S.: Porous functionalized polymers enable generating and transporting hyperpolarized mixtures of metabolites, *Nat Commun*, 12, 4695, <https://doi.org/10.1038/s41467-021-24279-2>, 2021.
- 665 Elliott, S. J., Stern, Q., Ceillier, M., El Daraï, T., Cousin, S. F., Cala, O., and Jannin, S.: Practical dissolution dynamic nuclear polarization, *Progress in Nuclear Magnetic Resonance Spectroscopy*, 126–127, 59–100, <https://doi.org/10.1016/j.pnmrs.2021.04.002>, 2021.
- Emwas, A.-H., Roy, R., McKay, R. T., Tenori, L., Saccenti, E., Gowda, G. A. N., Raftery, D., Alahmari, F., Jaremko, L., Jaremko, M., and Wishart, D. S.: NMR Spectroscopy for Metabolomics Research, *Metabolites*, 9, 123, <https://doi.org/10.3390/metabo9070123>, 2019.
- 670 Eshuis, N., Hermkens, N., van Weerdenburg, B. J. A., Feiters, M. C., Rutjes, F. P. J. T., Wijmenga, S. S., and Tessari, M.: Toward Nanomolar Detection by NMR Through SABRE Hyperpolarization, *J. Am. Chem. Soc.*, 136, 2695–2698, <https://doi.org/10.1021/ja412994k>, 2014.
- Frahm, A. B., Jensen, P. R., Ardenkjær-Larsen, J. H., Yigit, D., and Lerche, M. H.: Stable isotope resolved metabolomics classification of prostate cancer cells using hyperpolarized NMR data, *Journal of Magnetic Resonance*, 316, 106750, <https://doi.org/10.1016/j.jmr.2020.106750>, 2020.
- 675 Frahm, A. B., Hill, D., Katsikis, S., Andreassen, T., Ardenkjær-Larsen, J. H., Bathen, T. F., Moestue, S. A., Jensen, P. R., and Lerche, M. H.: Classification and biomarker identification of prostate tissue from TRAMP mice with hyperpolarized ^{13}C -SIRA, *Talanta*, 235, 122812, <https://doi.org/10.1016/j.talanta.2021.122812>, 2021.
- Giraudeau, P.: NMR-based metabolomics and fluxomics: developments and future prospects, *Analyst*, 145, 2457–2472, <https://doi.org/10.1039/D0AN00142B>, 2020.
- 680 Giraudeau, P., Shrot, Y., and Frydman, L.: Multiple Ultrafast, Broadband 2D NMR Spectra of Hyperpolarized Natural Products, *J. Am. Chem. Soc.*, 131, 13902–13903, <https://doi.org/10.1021/ja905096f>, 2009.
- Grotti, M., Soggia, F., Ardini, F., and Frache, R.: Determination of sub-nanomolar levels of iron in sea-water using reaction cell inductively coupled plasma mass spectrometry after $\text{Mg}(\text{OH})_2$ coprecipitation, *J. Anal. At. Spectrom.*, 24, 522, <https://doi.org/10.1039/b818236a>, 2009.
- 685 Guduff, L., Kurzbach, D., van Heijenoort, C., Abergel, D., and Dumez, J.-N.: Single-Scan ^{13}C Diffusion-Ordered NMR Spectroscopy of DNP-Hyperpolarised Substrates, *Chem. Eur. J.*, 23, 16722–16727, <https://doi.org/10.1002/chem.201703300>, 2017.

- 690 Guduff, L., Berthault, P., van Heijenoort, C., Dumez, J., and Huber, G.: Single-Scan Diffusion-Ordered NMR Spectroscopy of SABRE-Hyperpolarized Mixtures, *ChemPhysChem*, 20, 392–398, <https://doi.org/10.1002/cphc.201800983>, 2019.
- Hayashi, Y., Puzenko, A., Balin, I., Ryabov, Y. E., and Feldman, Y.: Relaxation Dynamics in Glycerol–Water Mixtures. 2. Mesoscopic Feature in Water Rich Mixtures, *J. Phys. Chem. B*, 109, 9174–9177, <https://doi.org/10.1021/jp050425d>, 2005.
- 695 Ivanov, K. L., Petrova, M. V., Lukzen, N. N., and Sagdeev, R. Z.: Separation of integral and multiplet nuclear polarization by means of spin echo magnetization phase analysis, *Dokl Phys Chem*, 427, 121–124, <https://doi.org/10.1134/S0012501609070021>, 2009.
- Jähnig, F., Himmler, A., Kwiatkowski, G., Däpp, A., Hunkeler, A., Kozerke, S., and Ernst, M.: A spin-thermodynamic approach to characterize spin dynamics in TEMPO-based samples for dissolution DNP at 7 T field, *Journal of Magnetic Resonance*, 303, 91–104, <https://doi.org/10.1016/j.jmr.2019.04.012>, 2019.
- 700 Jannin, S., Dumez, J.-N., Giraudeau, P., and Kurzbach, D.: Application and methodology of dissolution dynamic nuclear polarization in physical, chemical and biological contexts, *Journal of Magnetic Resonance*, 305, 41–50, <https://doi.org/10.1016/j.jmr.2019.06.001>, 2019.
- 705 Katsikis, S., Marin-Montesinos, I., Pons, M., Ludwig, C., and Günther, U. L.: Improved Stability and Spectral Quality in Ex Situ Dissolution DNP Using an Improved Transfer Device, *Appl Magn Reson*, 46, 723–729, <https://doi.org/10.1007/s00723-015-0680-5>, 2015.
- Kaushik, M., Lingua, H., Stevanato, G., Elokova, M., Lelli, M., Lesage, A., and Ouari, O.: Trehalose matrices for high temperature dynamic nuclear polarization enhanced solid state NMR, *Phys. Chem. Chem. Phys.*, 10.1039/D2CP00970F, <https://doi.org/10.1039/D2CP00970F>, 2022.
- 710 Kim, J. W., Ryu, S. H., Kim, S., Lee, H. W., Lim, M., Seong, S. J., Kim, S., Yoon, Y.-R., and Kim, K.-B.: Pattern Recognition Analysis for Hepatotoxicity Induced by Acetaminophen Using Plasma and Urinary ¹H NMR-Based Metabolomics in Humans, *Anal. Chem.*, 85, 11326–11334, <https://doi.org/10.1021/ac402390q>, 2013.
- Kiryutin, A. S., Sauer, G., Tietze, D., Brodrecht, M., Knecht, S., Yurkovskaya, A. V., Ivanov, K. L., Avrutina, O., Kolmar, H., and Buntkowsky, G.: Ultrafast Single-Scan 2D NMR Spectroscopic Detection of a PHIP-Hyperpolarized Protease Inhibitor, *Chem. Eur. J.*, 25, 4025–4030, <https://doi.org/10.1002/chem.201900079>, 2019.
- 715 Köckenberger, W.: Dissolution Dynamic Nuclear Polarization, in: *eMagRes*, edited by: Harris, R. K. and Wasylshen, R. L., John Wiley & Sons, Ltd, Chichester, UK, 161–170, <https://doi.org/10.1002/9780470034590.emrstm1311>, 2014.
- 720 Kouřil, K., Kouřilová, H., Bartram, S., Levitt, M. H., and Meier, B.: Scalable dissolution-dynamic nuclear polarization with rapid transfer of a polarized solid, *Nat Commun*, 10, 1733, <https://doi.org/10.1038/s41467-019-09726-5>, 2019.
- Kouřil, K., Gramberg, M., Jurkutat, M., Kouřilová, H., and Meier, B.: A cryogen-free, semi-automated apparatus for bullet-dynamic nuclear polarization with improved resolution, *Magn. Reson.*, 2, 815–825, <https://doi.org/10.5194/mr-2-815-2021>, 2021.
- 725 Kress, T., Che, K., Epasto, L. M., Kozak, F., Olsen, G. L., Selimovic, A., and Kurzbach, D.: A novel sample handling system for dissolution dynamic nuclear polarization experiments, *Hyperpolarization/Instrumentation*, <https://doi.org/10.5194/mr-2021-12>, 2021.
- Leavesley, A., Wilson, C. B., Sherwin, M., and Han, S.: Effect of water/glycerol polymorphism on dynamic nuclear polarization, *Phys. Chem. Chem. Phys.*, 20, 9897–9903, <https://doi.org/10.1039/C8CP00358K>, 2018a.
- 730 Leavesley, A., Wilson, C. B., Sherwin, M., and Han, S.: Effect of water/glycerol polymorphism on dynamic nuclear polarization, *Phys. Chem. Chem. Phys.*, 20, 9897–9903, <https://doi.org/10.1039/C8CP00358K>, 2018b.

- Leon Swisher, C., Koelsch, B., Sukumar, S., Sriram, R., Santos, R. D., Wang, Z. J., Kurhanewicz, J., Vigneron, D., and Larson, P.: Dynamic UltraFast 2D EXchange Spectroscopy (UF-EXSY) of hyperpolarized substrates, *Journal of Magnetic Resonance*, 257, 102–109, <https://doi.org/10.1016/j.jmr.2015.05.011>, 2015.
- 735 Lerche, M. H., Yigit, D., Frahm, A. B., Ardenkjær-Larsen, J. H., Malinowski, R. M., and Jensen, P. R.: Stable Isotope-Resolved Analysis with Quantitative Dissolution Dynamic Nuclear Polarization, *Anal. Chem.*, 90, 674–678, <https://doi.org/10.1021/acs.analchem.7b02779>, 2018.
- Li, Y., Bouza, M., Wu, C., Guo, H., Huang, D., Doron, G., Temenoff, J. S., Stecenko, A. A., Wang, Z. L., and Fernández, F. M.: Sub-nanoliter metabolomics via mass spectrometry to characterize volume-limited samples, *Nat Commun*, 11, 5625, <https://doi.org/10.1038/s41467-020-19444-y>, 2020.
- 740 Liem-Nguyen, V., Bouchet, S., and Björn, E.: Determination of Sub-Nanomolar Levels of Low Molecular Mass Thiols in Natural Waters by Liquid Chromatography Tandem Mass Spectrometry after Derivatization with *p* - (Hydroxymercuri) Benzoate and Online Preconcentration, *Anal. Chem.*, 87, 1089–1096, <https://doi.org/10.1021/ac503679y>, 2015.
- 745 Liu, Y., Huang, R., Liu, L., Peng, J., Xiao, B., Yang, J., Miao, Z., and Huang, H.: Metabonomics study of urine from Sprague–Dawley rats exposed to Huang-yao-zi using ¹H NMR spectroscopy, *Journal of Pharmaceutical and Biomedical Analysis*, 52, 136–141, <https://doi.org/10.1016/j.jpba.2009.12.026>, 2010.
- Lloyd, L. S., Adams, R. W., Bernstein, M., Coombes, S., Duckett, S. B., Green, G. G. R., Lewis, Richard. J., Mewis, R. E., and Sleight, C. J.: Utilization of SABRE-Derived Hyperpolarization To Detect Low-Concentration Analytes via 1D and 2D NMR Methods, *J. Am. Chem. Soc.*, 134, 12904–12907, <https://doi.org/10.1021/ja3051052>, 2012.
- 750 Milani, J., Vuichoud, B., Bornet, A., Miéville, P., Mottier, R., Jannin, S., and Bodenhausen, G.: A magnetic tunnel to shelter hyperpolarized fluids, *Review of Scientific Instruments*, 86, 024101, <https://doi.org/10.1063/1.4908196>, 2015.
- Mishkovsky, M. and Frydman, L.: Progress in Hyperpolarized Ultrafast 2D NMR Spectroscopy, *ChemPhysChem*, 9, 2340–2348, <https://doi.org/10.1002/cphc.200800461>, 2008.
- Overall, S. A. and Barnes, A. B.: Biomolecular Perturbations in In-Cell Dynamic Nuclear Polarization Experiments, *Front. Mol. Biosci.*, 8, 743829, <https://doi.org/10.3389/fmolb.2021.743829>, 2021.
- Plainchont, B., Berruyer, P., Dumez, J.-N., Jannin, S., and Giraudeau, P.: Dynamic Nuclear Polarization Opens New Perspectives for NMR Spectroscopy in Analytical Chemistry, *Anal. Chem.*, 90, 3639–3650, <https://doi.org/10.1021/acs.analchem.7b05236>, 2018.
- 760 Puzenko, A., Hayashi, Y., Ryabov, Y. E., Balin, I., Feldman, Y., Kaatze, U., and Behrends, R.: Relaxation Dynamics in Glycerol–Water Mixtures: I. Glycerol-Rich Mixtures, *J. Phys. Chem. B*, 109, 6031–6035, <https://doi.org/10.1021/jp0445122>, 2005.
- Singh, K., Jacquemmoz, C., Giraudeau, P., Frydman, L., and Dumez, J.-N.: Ultrafast 2D ¹H–¹H NMR spectroscopy of DNP-hyperpolarised substrates for the analysis of mixtures, *Chem. Commun.*, 57, 8035–8038, <https://doi.org/10.1039/D1CC03079E>, 2021a.
- 765 Singh, K., Jacquemmoz, C., Giraudeau, P., Frydman, L., and Dumez, J.-N.: Ultrafast 2D ¹H–¹H NMR spectroscopy of DNP-hyperpolarised substrates for the analysis of mixtures, *Chem. Commun.*, 57, 8035–8038, <https://doi.org/10.1039/D1CC03079E>, 2021b.
- Stern, Q., Cousin, S. F., Mentink-Vigier, F., Pinon, A. C., Elliott, S. J., Cala, O., and Jannin, S.: Direct observation of hyperpolarization breaking through the spin diffusion barrier, *Sci. Adv.*, 7, eabf5735, <https://doi.org/10.1126/sciadv.abf5735>, 2021.
- 770 Strickland, J., Zang, Q., Paris, M., Lehmann, D. M., Allen, D., Choksi, N., Matheson, J., Jacobs, A., Casey, W., and Kleinstreuer, N.: Multivariate models for prediction of human skin sensitization hazard: Multivariate models for prediction of human skin sensitization hazard, *J. Appl. Toxicol.*, 37, 347–360, <https://doi.org/10.1002/jat.3366>, 2017.

- 775 Tran, N. T., Mentink-Vigier, F., and Long, J. R.: Dynamic Nuclear Polarization of Biomembrane Assemblies, *Biomolecules*, 10, 1246, <https://doi.org/10.3390/biom10091246>, 2020.
- Wang, B., Goodpaster, A. M., and Kennedy, M. A.: Coefficient of variation, signal-to-noise ratio, and effects of normalization in validation of biomarkers from NMR-based metabonomics studies, *Chemometrics and Intelligent Laboratory Systems*, 128, 9–16, <https://doi.org/10.1016/j.chemolab.2013.07.007>, 2013.
- 780 Weber, E. M. M., Sicoli, G., Vezin, H., Frébourg, G., Abergel, D., Bodenhausen, G., and Kurzbach, D.: Sample Ripening through Nanophase Separation Influences the Performance of Dynamic Nuclear Polarization, *Angew. Chem. Int. Ed.*, 57, 5171–5175, <https://doi.org/10.1002/anie.201800493>, 2018.
- Wishart, D. S.: Quantitative metabolomics using NMR, *TrAC Trends in Analytical Chemistry*, 27, 228–237, <https://doi.org/10.1016/j.trac.2007.12.001>, 2008.
- 785 Zhang, S., Nagana Gowda, G. A., Asiago, V., Shanaiah, N., Barbas, C., and Raftery, D.: Correlative and quantitative ¹H NMR-based metabolomics reveals specific metabolic pathway disturbances in diabetic rats, *Analytical Biochemistry*, 383, 76–84, <https://doi.org/10.1016/j.ab.2008.07.041>, 2008.
- Zhang, S., Nagana Gowda, G. A., Ye, T., and Raftery, D.: Advances in NMR-based biofluid analysis and metabolite profiling, *Analyst*, 135, 1490, <https://doi.org/10.1039/c000091d>, 2010.